

Ride® Custom 2 Cushion and Custom Back From Scan, Itemized Order Form

Download this form and open in Adobe for optimum functionality

Client's First and Last Name _____

Please be sure client's name is consistent on all correspondence: order forms, purchase order, etc.

☐ Ride Custom 2 Cushion (RCC200)

Shape provided via:

☐ RideWorks® Scan

☐ Other _____

☐ Ride Custom Back (RCB200)

Shape provided via:

☐ RideWorks® Scan

☐ Other _____

Note: If you wish to order using our made from measurements option, please visit www.ridedesigns.com/order-forms/ and choose the appropriate made-from-measurements order form.

Account # _____
PO # _____
Date _____ SO# _____
SN# _____

Date of shape capture: _____

*Internal management of personal information is HIPAA compliant.

General Information

Supplier _____

Ride Certified Practitioner Name _____

Address _____

City _____ State _____ Zip _____

Phone # _____ Email _____

Ship to (if different from above)

NOTE: Ride Custom Systems must be fitted by a Ride Certified Provider. Therefore we will not drop ship to end users.

Address _____

City _____ State _____ Zip _____

Phone # _____ Email _____

Referral Source

Facility Name _____

Clinician Name _____

Phone # _____ Email _____

Ride® Custom 2 Cushion and Custom Back From Scan Itemized Order Form

Client First and Last Name _____

Client Information

WARNING: Caution should be exercised when capturing shapes in Ride Simulators for people with osteoporosis, bone cancer, history of pathological fracture, osteogenesis imperfecta, or any brittle bone condition.

Sex: ☐ M ☐ F Diagnosis _____

Does client have:

☐ Current tissue injury? Location _____ Stage _____

☐ History of tissue injury? Location _____ Stage _____

Height _____ Weight _____

Client Measurements

A. Trochanters _____"

B. Leg length L _____" R _____"

C. Iliac Crest _____"

D. Mid-Thorax _____"

E. Axilla _____"

F. A-P Mid-Thorax _____"

G. Top of Iliac Crest L _____" R _____"


H. Axilla height L _____" R _____"

I. Top of shoulder L _____" R _____"

J. Knee to heel _____"

K. Top of head _____"


L. A-P abdomen _____"

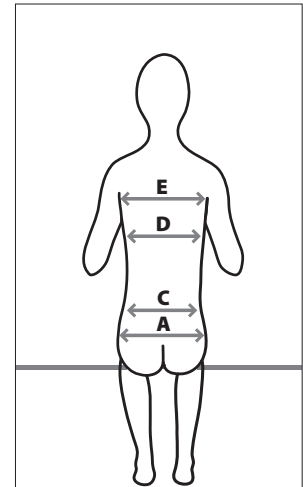


Mobility Base Specifications

Wheelchair Make _____ Model _____

Frame Width _____" Depth _____"

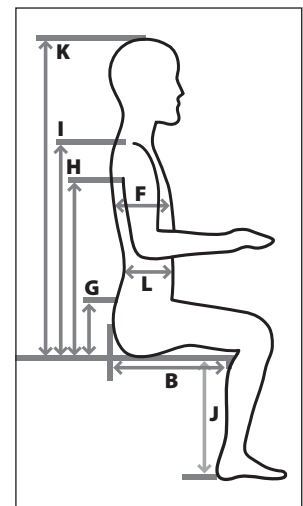

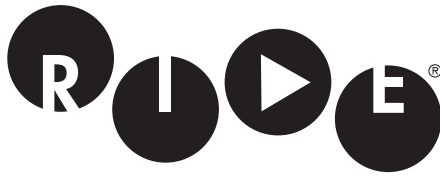

Ride[®] Custom 2 Cushion from Scan Itemized Order Form

Client First and Last Name _____

Prices effective January 13, 2025.

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Ride Custom 2 Cushion Includes 2 CAM [®] Wedges Medicare HCPCS Code E2609	RCC200	\$1960.00
☐ Ride Custom 2 Cushion with commode opening and solid seat pan without cover	RCC200-C	\$1960.00

Shape Capture Process (please check one)

- ☐ Bead Bag
Indicate Shape Capture Base size used:
☐ Small (Blue) ☐ Medium (White)
☐ Large (Red) ☐ None
- ☐ Shape Capture Base is Wedged Up _____"
☐ Front ☐ Rear
☐ Left Side ☐ Right Side
- ☐ Build wedge into cushion per simulation RCC2-WS \$ 183.00
☐ Do not build wedge into cushion
- ☐ Scan of existing cushion (insert existing cushion measurements below)
Length L _____" R _____" Rear width _____" Front width _____"
Height at the following corners: Front L _____" Front R _____" Rear L _____" Rear R _____"
(Heights are not guaranteed if the cushion being scanned is a discontinued product.)

Is the existing cushion used on a sling seat? ☐ Yes ☐ No

(If yes, please note the new cushion will be made with a flat bottom. If the cushion being duplicated has a rounded bottom from use in the sling, this may result in height differences between the existing cushion and new cushion. Add the Bevel Cut option if the new cushion will be used on a sling seat.)

Resting Posture of Pelvis in Ride Shape Capture

☐ Neutral ☐ Posterior ☐ Anterior

1. Photos and Scan

Using RideWorks? Use RideWorks app to:

- ☐ Photograph front and both sides of client during shape capture.
- ☐ Photograph captured shape.
- ☐ Scan captured shape.
- ☐ Take any and all additional photos that may help.

Not using RideWorks? Include:

- ☐ Photograph of front and both sides of client during shape capture.
- ☐ Photograph of captured shape.

Page 3

Continue on page 4

* All prices are in U.S. dollars.

RideWorks® Custom 2 Cushion and Custom Back From Scan Itemized Order Form

Client First and Last Name _____

2. Foam Options

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Standard Foam (max. weight 250 lbs.)	RCC2-SF	Standard
☐ Firm Foam (max. weight 300 lbs.)	RCC2-FF	\$ 138.00
☐ Standard Foam with front cushion reinforcement	RCC2-SF-CR	\$ 326.00
☐ Firm Foam with front cushion reinforcement	RCC2-FF-CR	\$ 490.00

3. Cushion/Wheelchair Interface (Flat bottom for solid seat is standard.)

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Bevel Cut Modification for sling seat	RCC2-BC	\$ 156.00
☐ Drop Seat Modification, 1" drop	RCC2-WC003	\$ 156.00
☐ Custom Mounting Platform ABS platform with indexing tabs to ensure correct placement of cushion on seat (not compatible with bevel cut modification or drop seat modification)	RCC2-CMP	\$ 495.00

4. Cushion Width (Actual cushion width will be 1/4" less than specified.)

Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.

Item	Part Number	Mfr. Sugg. Retail Price*
Standard ☐ 10" ☐ 11" ☐ 12" ☐ 13" ☐ 14" ☐ 15" (width) ☐ 16" ☐ 17" ☐ 18" ☐ 19" ☐ 20"	RCC2-____	No charge
Extra large width: (The selection of Firm Foam RCC2-FF is strongly recommended) ☐ 21" ☐ 22" ☐ 23" ☐ 24" (width)	RCC2-W____	\$ 162.00
☐ Tapered width Back width _____" Front width _____"	RCC2-CWTW	\$ 162.00

**NOTE: For cushion widths
greater than 24,"
please call for a quote.**


5. Cushion Length (IMPORTANT: Specify cushion length relative to front of Shape Capture Base as shown.)

Measure from front of Shape Capture Base to establish cushion length.

Note: Cushion must not exceed wheelchair dimensions by more than 1" in any direction.

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Equal to Shape Capture Base length	RCC2-CLAC	Standard
Symmetrical Length ☐ Add _____" to Shape Capture Base length ☐ Subtract _____" to Shape Capture Base length	RCC2-CLSL	No charge
Asymmetrical Length		\$ 156.00
LEFT ☐ Equal to Shape Capture Base length ☐ Add _____" to Shape Capture Base length ☐ Subtract _____" to Shape Capture Base length	RCC2-CLALL	
RIGHT ☐ Equal to Shape Capture Base length ☐ Add _____" to Shape Capture Base length ☐ Subtract _____" from Shape Capture Base length	RCC2-CLALR	


Missed this step? Indicate desired length
of cushion on each side L _____" R _____"

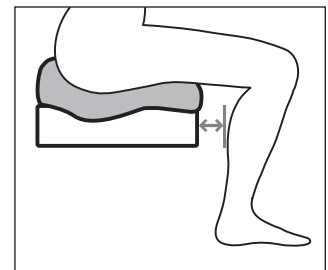

RideWorks® Custom 2 Cushion and Custom Back From Scan Itemized Order Form
Client First and Last Name _____

6. Modifications


Item	Part Number	Mfr. Sugg. Retail Price*
☐ 1" undercut	RCC2-UC1	\$ 87.00
☐ Front rigging notches _____ " W x _____ " D x _____ " H	RCC2-WCFR	\$ 100.00
☐ Ventilation channel	RCC2-VC	\$ 184.00

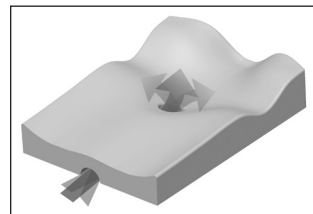

Custom ventilation channel helps manage heat and moisture.

7. Sitting Height

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Targeted final front cushion height (see diagrams at right) Height: L leg _____ " R leg _____ " NOTE: This final height is not guaranteed. Results are dependent upon the accuracy of the captured shape. Height does not include cover thickness.	RCC2-SHTH	No charge
☐ As captured	RCC2-SHAC	Standard
☐ Increase overall height _____ "	RCC2-SHIH	\$ 183.00
☐ As low as possible NOTE: Cushion height will be lowered to achieve minimum foam thickness in I.T. well. This may not result in a lower final front cushion height.	RCC2-SHDH	\$ 183.00

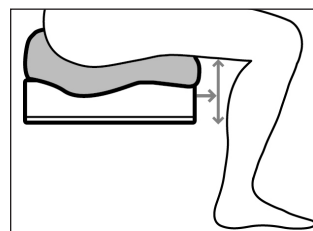

For targeted cushion height: at the projected cushion length, measure from the bottom of the shape capture base up to the underside of the leg with the feet properly positioned on the footplate(s).

8. Cushion Contour

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Off-load bony prominences Off-loads bony prominences and enhances loading of areas tolerant of pressure and shear for best skin protection, postural control and microclimate.	RCC2-OBP	Standard
☐ Reticulated foam well insert kit For gentle support to bony prominences and to maintain a high level of microclimate management. ⚠ ONE SIZE: Must be trimmed in field to fit.	RCC2-WI	\$ 57.00
☐ Full contact Cushion manufactured as captured (compromises air flow and microclimate management at bony prominences). ⚠ WARNING: Full contact is not recommended for users at high risk of skin breakdown.	RCC2-FC	No charge



Determine targeted front of cushion height (front view).

9. Thigh/Femoral Support

Item	Part Number	Mfr. Sugg. Retail Price*
Medial Thigh Support If no selection is made, the medial thigh support will be manufactured as captured.		
☐ As captured	RCC2-MTAC	Standard
☐ Eliminate	RCC2-MTE	No charge
☐ Increase _____" (maximum 3" total height from bottom of leg trough)	RCC2-MTI	\$ 139.00
☐ Decrease _____"	RCC2-MTD	No charge
☐ Decrease as marked with line on Shape Capture Bag	RCC2-MTM	No charge

Lateral Thigh Support

LEFT

☐ As captured	RCC2-LTAC	Standard
☐ Eliminate	RCC2-LTEL	No charge
☐ Increase _____" (maximum 3" total height from bottom of leg trough)	RCC2-LTIL	\$ 139.00
☐ Decrease _____"	RCC2-LTDL	No charge
☐ Decrease as marked with line on Shape Capture Bag	RCC2-LTML	No charge

RIGHT

☐ As captured	RCC2-LTAC	Standard
☐ Eliminate	RCC2-LTER	No charge
☐ Increase _____" (maximum 3" total height from bottom of leg trough)	RCC2-LTIR	\$ 139.00
☐ Decrease _____"	RCC2-LTDR	No charge
☐ Decrease as marked with line on Shape Capture Bag	RCC2-LTMR	No charge

10. Covers

Item	Part Number	Mfr. Sugg. Retail Price*
☐ One breathable spacer fabric zip cover included		Standard
☐ Spandex layer over spacer fabric	RCC2-SP	\$ 95.00
☐ Two-layer spacer fabric Soft Fit	RCC2-EM2	\$ 172.00
☐ Additional breathable spacer fabric zip cover	RCC2-CBZA ____ (width)	\$ 249.00
☐ Spandex layer over spacer fabric	RCC2-SP	\$ 95.00
☐ Two-layer spacer fabric Soft Fit	RCC2-EM2	\$ 172.00
☐ Outer incontinent resistant cover Note: Only recommended for chronically incontinent clients. Does not replace spacer fabric cover.	RCC2-IC	\$ 299.00
☐ Inner incontinent resistant cover Note: Only recommended for chronically incontinent clients. Does not replace spacer fabric cover.	RCC2-INICA	\$ 299.00

11. Additional Custom Cushion Accessories/Items

Item	Part Number	Mfr. Sugg. Retail Price*	Qty
1" / 3cm Cushion Orientation Wedge (These wedges are loose. To order a built-in wedge please see page 3)			
☐ For 14" / 36cm cushion widths	RCC2-OW-1414	\$ 96.00	
☐ For 15" / 38cm and 16" / 41cm cushion width	RCC2-OW-1616	\$ 96.00	
☐ For 17" / 43cm and 18" / 46cm cushion widths	RCC2-OW-1816	\$ 96.00	
☐ For 19" / 48cm and 20" / 51cm cushion widths	RCC2-OW-2016	\$ 96.00	
Wedge to be used: (select one)			
☐ Outside cover			
☐ Inside cover			
If inside cover, thick edge of the wedge to be placed:			
☐ Back of cushion			
☐ Front of cushion			
☐ Left side of cushion			
☐ Right side of cushion			
☐ Ride CAM® Wedge Kit**	RCC2-WK	\$ 45.00	


12. Growth

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Growth Kit	RCC2-DGK	\$ 307.00
Provides for one growth adjustment, including a new cover, during two year warranty period. Width and/or length, and/or height only. Changes in pelvic alignment and body shape can not be accommodated through growth adjustment. (This option requires shipping cushion to Ride Designs with RA.)		
Total:		_____

Special Instructions or Comments

NOTE: May affect price; call to request quote.

* All prices are in U.S. dollars.
** One size fits all. Trim in field for correct fit.

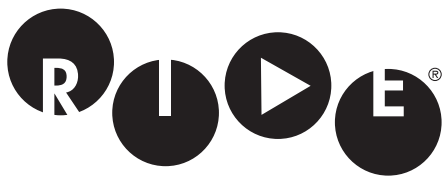

Ride® Custom Back from Scan Itemized Order Form

Client First and Last Name _____

Prices effective January 13, 2025.



► **Before transferring client from shape capture bag,** please complete the following...

PHOTOS of client in shape capture bag: ☐ Front view

☐ Side view

☐ Included in RideWorks® client files

☐ Emailed to customerservice@ridedesigns.com, with client name and provider information

☐ Attached

Trim lines; establish and mark on clear, outer shape capture bag:

☐ Back height

☐ Lateral support depth and height

☐ Mark distal laterals and indicate measurement between them.

► **Before scanning,** on the clear, outer shape capture bag (using a black permanent marker), draw trim lines and marks to draw the back as it should be manufactured, including:

☐ Arrow pointing upward, indicating top of back

☐ Soft relief areas to protect bony prominences

☐ Depth and height of the lateral trunk supports

☐ Measurement between marks on distal laterals

► **Important! If you're ordering a Ride Custom Back without a scan, please do not complete this order form. Please visit www.ridedesigns.com/order-forms/ and select the appropriate order form under "Made from Measurements Order Method."**

DID YOU SEND
PHOTOS?



Ride® Custom 2 Cushion and Custom Back from Scan Itemized Order Form

Client First and Last Name _____

1. Ride Custom Back Type


Item	Part Number	Mfr. Sugg. Retail Price*
☐ Ride Custom Back Medicare HCPCS Code E2617 Custom contoured seat back shell; choice of 1) ultra-breathable, 3D mesh liner, or 2) AccuSoft® foam liner; and spacer fabric cover. Note: if AccuSoft foam liner option is selected, Back comes with choice of spacer fabric cover or wipeable, and incontinence-proof cover.	RCB200	\$ 2529.00
☐ Ride Custom Back, for Commode Back Includes custom contoured seat back shell lined with 3D mesh liner and a shower-cap style cover.	RCB200-C	\$ 2529.00

2. Ride Custom Back Size

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Trunk width is ≤ 20"	RCB2-200R	\$ 0.00
☐ Trunk width is 21" - 24"	RCB2-200W	\$ 402.00

For widths greater than 24", pricing will be individually determined and quoted.

Targeted width from top of left lateral trimline (A) to top of right lateral trimline (B) _____"
(Providing this information will help us to ensure the finished product specs are accurate.)

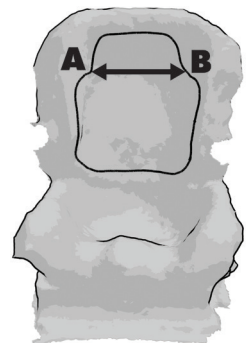

Ride® Custom 2 Cushion and Custom Back from Scan Itemized Order Form
Client First and Last Name _____

3. Ride Custom Back Hardware and Mounting

Item	Part Number	Mfr. Sugg. Retail Price*
------	-------------	--------------------------

Ride FlexLoc® Hardware

NOTE: Sections a, b, and c **MUST** have a selection.

a. Select Size and Quantity:

NOTE: Order the hardware size that matches the distance between mounting locations, not necessarily the wheelchair width. Mounting FlexLoc to Permobil® or Quantum® requires small FlexLoc mounting hardware with FlexLoc Adapter Plates from Ride Designs, Direct Backrest Frame from Permobil, or Aftermarket Back Interface from Quantum.

*WARNING! Two (2) sets of FlexLoc hardware are required if the client presents with any of the following:

- Weight exceeds 250 pounds
- Overall back height measurement (as measured to trim lines on bag) is greater than or equal to 28"
- Severe extensor tone, spasticity, etc.

☐ Single Set of Hardware

☐ Double Set of Hardware

☐ Small, mounting distance 10 - 14"

☐ Medium, mounting distance 15 - 18"

☐ Large, mounting distance 19 - 21"

☐ X-Large, mounting distance 22 - 24"

☐ Omit hardware

	Part Number	MSRP per set
	RCB2-FL-MS	\$ 649.00
	RCB2-FL-MM	\$ 649.00
	RCB2-FL-ML	\$ 649.00
	RCB2-FL-MX	\$ 649.00
	RCB2-200R-0	\$ 0.00

b. Select Mounting:

☐ Clamp Mount for round back canes

☐ Additional Mounting Clamps (pair)

NOTE: If ordering Double FlexLoc mounting hardware, two sets of mounting clamps are included.

☐ Quickie Sedeo Pro Interface Bracket

Mounts RCB200 to Quickie Sedeo Pro Power Seating System with recline.

☐ Quickie Sedeo Pro Advanced Interface Bracket

Mounts RCB200 to Quickie Sedeo Pro Advanced Power Seating System with recline.

• RCB2-QSIB and RCB2-QSAIB are not compatible with tilt-only Sedeo Pro Seating System. Mounting options for Sedeo seating without recline are available through Sunrise Medical Built-4-Me and require ordering Ride's FlexLoc Adapter Plate, below.

• RCB2-QSIB and RCB2-QSAIB are available as a single-mount option. Call for options if double hardware is needed on a Sedeo Pro seating system.

• Order small FlexLoc hardware and Quick Release attachment for use with RCB2-QSIB and RCB2-QSAIB.

• RCB2-QSIB and RCB2-QSAIB replace cane clamps.

☐ FlexLoc Adapter Plate

RCB2-FL-MCI-P1

No Charge

For mounting to Sedeo Pro seating systems without recline, and wheelchairs without round back canes, e.g. Permobil 3G, Invacare Tilt and Recline, or general surface mounting to existing back pans. This option replaces cane clamps.

☐ Fixed, non-removeable

RCB2-FL-FMI

Standard

☐ Quick Release Option


RCB2-FL-QR

\$ 107.00

NOTE: The Ride FlexLoc Mount can be interfaced with most any wheelchair configuration. Contact Ride Designs for a solution to your mounting challenge.



Ride FlexLoc Hardware on RCB200

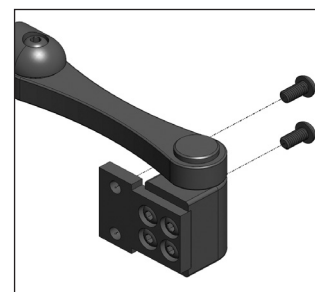

Adapter Plate



Quick Release Option

c. Select Attachment:

Ride® Custom 2 Cushion and Custom Back From Scan Itemized Order Form

Client First and Last Name _____

4. Foam Options

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Ultra-breathable 3D mesh liner	RCB2-SML	\$ 0.00
☐ Additional layer of 3D mesh liner (increases each lateral support thickness by ½")	RCB2-2SML	\$ 210.00
☐ AccuSoft foam liner (increases each lateral support thickness by ½" and may result in compromise of postural correction)	RCB2-FS	\$ 188.00
For AccuSoft option, select one cover:		
☐ Spacer fabric cover	RCB2-SFC	\$ 0.00
☐ Wipeable, incontinence-proof cover (Available for AccuSoft foam liner option only.)	RCB2-IC	\$ 0.00



Ultra-breathable foam liner



AccuSoft foam liner

5. Supplementary Padding, Reliefs, Dimensions

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Soft Fit Half-inch thick, breathable, reticulated foam liner for a softer feel.	RCB2-SF	\$ 443.00
☐ Complete back (including laterals) Increases each lateral support thickness by ½" and may result in compromise of postural correction.		
☐ Center only (excludes laterals)		
☐ Enhanced relief Typically used for improved protection and comfort at specific skeletal prominences such as rib humps and spinous processes.	RCB2-ERFP	\$ 389.00
— Draw desired location(s) and shape of relief on clear, outer shape capture bag.		

Axillary support pad

Typically used for distribution of corrective forces near the axilla on concave side of scoliosis.

☐ Left	RCB2-ASP-L	\$ 228.00
☐ Right	RCB2-ASP-R	\$ 228.00

Extended depth lateral thoracic support

☐ Extend LEFT lateral thoracic support _____" forward of reference line.	RCB2-EDLTS-L	\$ 378.00
☐ Extend RIGHT lateral thoracic support _____" forward of reference line.	RCB2-EDLTS-R	\$ 378.00
— Mark reference line(s) on clear, outer shape capture bag.		

Extended height lateral thoracic support

☐ Increase LEFT lateral thoracic support _____" above reference line.	RCB2-EHLTS-L	\$ 249.00
☐ Increase RIGHT lateral thoracic support _____" above reference line.	RCB2-EHLTS-R	\$ 249.00

Extended back height

☐ Extend back height _____" above reference line.	RCB2-EBH	\$ 378.00
— Mark reference line(s) on clear, outer shape capture bag.		

☐ Reinforced lateral thoracic supports

RCB2-RLTS \$ 495.00

Note: No longer automatically required for lateral supports more than 6" deep. It is not possible to modify the width of lateral supports on the RCB200 by bending or flaring the lateral reinforcement. Width adjustments must be made by heating the back shell.

☐ Vertical back reinforcement	RCB2-RBS	\$ 365.00
--	----------	-----------

PHOTOS??
JUST CHECKING.

Minimum back height requirements for headrest accessory use		
Headrest Type	with Single Hardware	with Double Hardware
None	7"/0.178m	12"/0.330m
Universal Headrest Mounting Plate	11.5"/0.292m	18"/0.457m
Integrated Headrest/Accessories Mount	9.5"/0.241m	15.5"/0.394m
NOTE: Measure back height from top trimline to bottom trimline.		

Ride® Custom 2 Cushion and Custom Back From Scan Itemized Order Form

Client First and Last Name _____

6. Accessories

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Universal headrest mounting plate, installed Note: Will be installed midline, top of back, unless otherwise marked on clear, outer shape capture bag.	RCB2-UHMP	\$ 210.00
☐ Integrated headrest/accessories mount Note: May be mounted to FlexLoc vertical track if back height is not sufficient for an integrated mount.	RCB2-AM	\$ 312.00
☐ Headrest Mount Extension Allows for clearance between the headrest post and the FlexLoc hardware	RCB2- HME	\$ 76.00
☐ Abdominal panel attachment plate only Included when abdominal support panel is ordered below, but also a great option on its own for mounting a chest harness or belts.	RCB2-APAP	\$ 224.00
☐ Shoulder harness guides, pair, loose	RCB2-SHG	\$ 127.00
☐ Shoulder harness guides, pair, installed Note: Mark location on clear, outer shape capture bag.	RCB2-SHGI	\$ 216.00

Privacy flap

Covers gap between cushion and back support.

Size

- | | | |
|--|----------|-----------|
| ☐ Small — fits wheelchair widths less than 14" | RCB2-PFS | \$ 171.00 |
| ☐ Medium — fits wheelchair widths 15 - 17" | RCB2-PFM | \$ 171.00 |
| ☐ Large — fits wheelchair widths 18" and larger | RCB2-PFL | \$ 171.00 |

Abdominal support panel


Recommended for clients with anterior pelvic tendencies.

Size

- | | | |
|--|-----------|-----------|
| ☐ Small — height 4" (two straps) | RCB2-AP-4 | \$ 449.00 |
| ☐ Medium — height 6" (three straps) | RCB2-AP-6 | \$ 449.00 |
| ☐ Large — height 8" (three straps) | RCB2-AP-8 | \$ 449.00 |



Universal Headrest Mounting Plate.

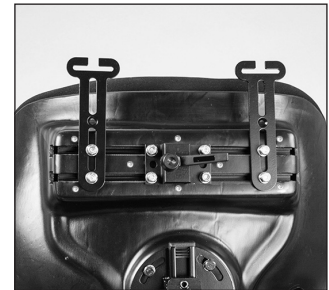

Integrated Headrest/Accessories Mount with Shoulder Harness Guides and headrest mount installed.




Privacy flap covers the space between the cushion and back support.

7. Covers

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Additional breathable cover	RCB2-SFCA	\$ 422.00
☐ Additional wipeable, incontinence-proof cover	RCB2-ICA	\$ 422.00

8. Growth

Item	Part Number	Mfr. Sugg. Retail Price*
☐ Growth Kit Provides for one growth adjustment, including a new cover, during two year warranty period. Width and/or height only. Changes in spinal alignment and body shape can not be accommodated through growth adjustment.	RCB2-DGK	\$ 563.00

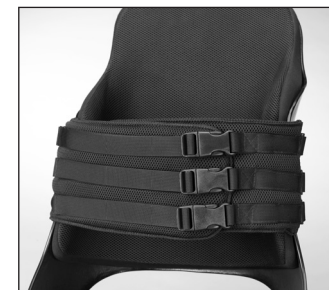

Abdominal Support Panel.

Special Instructions or Comments

NOTE: May affect price; call to request quote.

We offer a generous fit and function guarantee and a two year warranty for all our custom products. Details can be found on our website at www.ridedesigns.com.

PHOTOS??
THEY MUST BE
HERE SOMEWHERE.



Ride Designs®
a branch of Aspen Seating, LLC



toll-free 866.781.1633
phone 303.781.1633
fax 303.781.1722

www.ridedesigns.com
customerservice@ridedesigns.com